

## Case History 5 - PAD Plus in Periodontics (3)

Dr Tobias Wieser

Use of PAD following curettage




Deep pocket on mesial aspect of 23



Cleaning of pocket using scaler



After mechanical debridement, the photosensitiser is syringed into the pocket and left for 60 seconds. The periodontal tip attached to the light guide is then inserted into the depth of the pocket. The profile of the tip (matched in size and shape to a periodontal ) probe permits the correct placement without

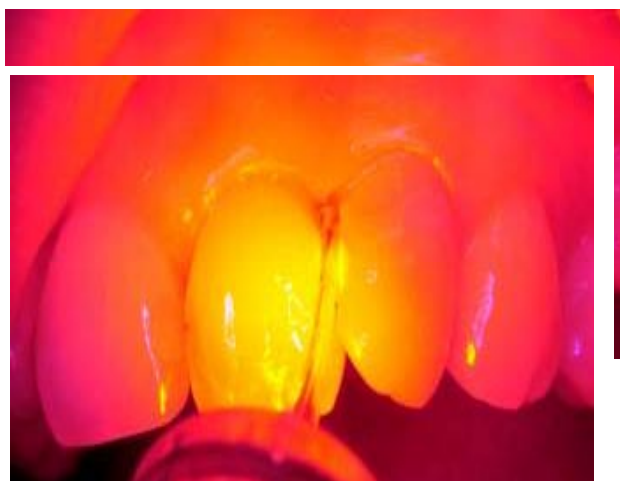

The light is activated for 60 seconds and treatment is complete